

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXD-0007
Location: KEYPORT POLICE
Calibration File No.: 00620 **Calib. Date:** 08/14/2015 **Calib. No.:** 00020
Certification File No.: 00621 **Cert. Date:** 08/14/2015 **Cert. No.:** 00016
Linearity File No.: 00622 **Lin. Date:** 08/14/2015 **Lin. No.:** 00016
Solution File No.: 00641 **Soln. Date:** 11/08/2015 **Soln. No.:** 00146
Sequential File No.: 00641 **File Date:** 11/08/2015

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDZK-0100
Control Solution %: 0.100% **Expires:** 12/31/2016
Solution Control Lot: 14L135 **Bottle No.:** 1244

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:43S		
Control 1 EC	0.099%	05:43S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	05:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:44S		
Control 2 EC	0.098%	05:45S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	05:45S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:45S		
Control 3 EC	0.098%	05:46S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	05:46S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:47S		

All tests within acceptable tolerance.

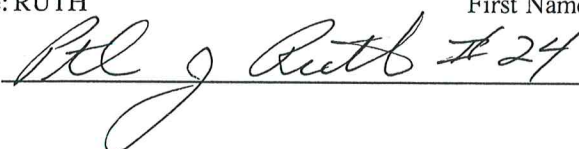
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: RUTH

First Name: JOSEPH

MI: H

Signature: 

Badge No.: 2224

Date: 11/08/2015